

**PCT**WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau

## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6: <b>G01N 21/86, 33/558, 33/543</b>	<b>A1</b>	(11) International Publication Number: <b>WO 95/13531</b>
		(43) International Publication Date: 18 May 1995 (18.05.95)

(21) International Application Number: PCT/EP94/03700

(22) International Filing Date: 8 November 1994 (08.11.94)

## (30) Priority Data:

93309053.2 12 November 1993 (12.11.93) EP

(34) Countries for which the regional or  
international application was filed: AT et al.

(71) Applicant: UNIPATH LIMITED [GB/GB]; Wade Road, Basingstoke, Hampshire RG24 0PW (GB).

(72) Inventors: CATT, Michael; 14 Brampton Close, Wellingborough, Northampton NN8 5XG (GB). MUNDILL, Paul, Henry, Charles; 44 Ashby Drive, Rushden, Northampton NN10 9HH (GB). PRIOR, Michael, Evans; 330 Newton Road, Rushden, Northampton NN10 0SY (GB).

(74) Agent: BUTLER, David, John; Unilever plc, Patent Division, Colworth House, Sharnbrook, Bedford MK44 1LQ (GB).

(81) Designated States: AM, AT, AU, BB, BG, BR, BY, CA, CH, CN, CZ, DE, DK, EE, ES, FI, GB, GE, HU, JP, KE, KG, KP, KR, KZ, LK, LR, LT, LU, LV, MD, MG, MN, MW, NL, NO, NZ, PL, PT, RO, RU, SD, SE, SI, SK, TJ, TT, UA, UZ, VN, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG), ARIPO patent (KE, MW, SD, SZ).


## Published

With international search report.

(54) Title: READING DEVICES FOR TESTSTRIPS

## (57) Abstract

A method of "reading" the result of an assay effected by concentrating a detectable material in a comparatively small zone of a carrier in the form of a strip, sheet or layer through the thickness of which electromagnetic radiation such as visible light is transmissible, wherein at least a portion of one face of the carrier is exposed to incident electromagnetic radiation which is substantially uniform across the entire portion, the portion including the small zone, and electromagnetic radiation emerging from the opposite face of the carrier is measured to determine the assay result. Preferably the radiation is diffuse light.

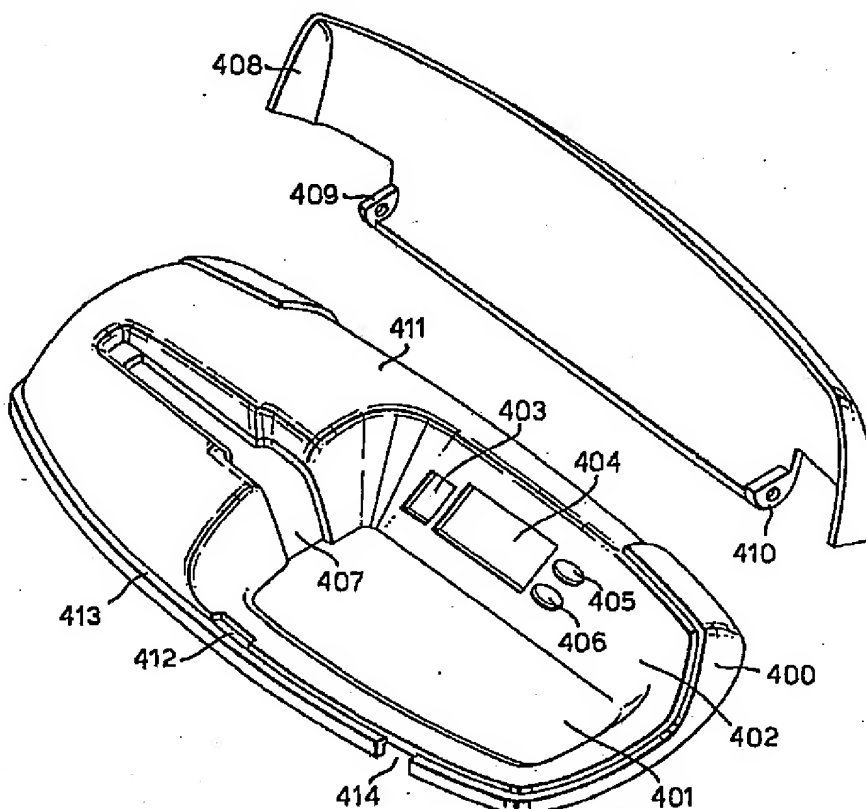

# INTERNATIONAL SEARCH REPORT

information on patent family members

International Application No

PCT/EP 94/03700

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP-A-0291194		FR-A- 2614423	28-10-88
		WO-A- 8808534	03-11-88
		GB-A- 2204398	09-11-88
		JP-A- 6180320	28-06-94
		JP-A- 6160388	07-06-94
		JP-T- 1503174	26-10-89
		AU-A- 1704992	27-08-92
		AU-A- 1705092	27-08-92

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/EP 94/03700

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP-A-0283285	21-09-88	JP-A- 63304143	12-12-88
EP-A-0492326	01-07-92	DE-A- 4041905 US-A- 5281395	02-07-92 25-01-94
EP-A-0165535	27-12-85	AU-B- 554849 AU-A- 4207685 CA-A- 1226453 DE-A- 3584042 JP-A- 61013136 US-A- 4755058	04-09-86 02-01-86 08-09-87 17-10-91 21-01-86 05-07-88
FR-A-2615953	02-12-88	JP-A- 63309845 US-A- 4931659	16-12-88 05-06-90
EP-A-0560411	15-09-93	AU-B- 626207 AU-A- 1622888 DE-D- 3887771 DE-T- 3887771 DE-U- 8805565 EP-A- 0291194 EP-A- 0560410 ES-T- 2050704 FR-A- 2614423 WO-A- 8808534 GB-A- 2204398 JP-A- 6180320 JP-A- 6160388 JP-T- 1503174 AU-A- 1704992 AU-A- 1705092	23-07-92 02-12-88 24-03-94 26-05-94 18-08-88 17-11-88 15-09-93 01-06-94 28-10-88 03-11-88 09-11-88 28-06-94 07-06-94 26-10-89 27-08-92 27-08-92
EP-A-0291194	17-11-88	AU-B- 626207 AU-A- 1622888 DE-D- 3887771 DE-T- 3887771 DE-U- 8805565 EP-A- 0560410 EP-A- 0560411 ES-T- 2050704	23-07-92 02-12-88 24-03-94 26-05-94 18-08-88 15-09-93 15-09-93 01-06-94

READING DEVICES FOR TESTSTRIPS

5 This invention relates to devices for reading the results of assays, to assay devices for use in conjunction with reading devices, and to methods using such devices.

10 An objective of the invention is to provide assay result reading devices and associated sample testing devices which can provide accurate quantitative assay information in a simple, quick and cost effective manner. Such devices can be used in a wide range of situations such as hospitals, clinics, doctors' offices, and the home. Depending on the circumstances, the analyte under investigation can also vary widely. Examples are infectious disease organisms or  
15 markers, metabolites in body fluids indicative of a change in the health or condition of a patient, and administrable or ingestible substances such as medicaments or drugs of abuse.

20 The invention is particularly, although not exclusively, concerned with assays which can be performed by comparatively untrained people and especially in the home.

25 Home-use assay devices such as pregnancy tests are now well established. In the case of a pregnancy test, which merely needs to provide the user with a "yes/no" result, the technology now available enables the assay result to be read easily by eye without the need for any ancillary equipment.

30 Home-use assays are intended primarily to detect physiological changes in the human body, with the objective of promoting the health, general well-being or lifestyle of the individual. The consumer is becoming increasingly  
35 health conscious, and the ability of the consumer to monitor his or her bodily functions is being encouraged. In some instances this can facilitate the interaction

## INTERNATIONAL SEARCH REPORT

Inter national Application No  
PCT/EP 94/03700

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	DATABASE WPI Week 8828, Derwent Publications Ltd., London, GB; AN 88-195635 & JP,A,63 134 953 (SHIMADZU SEISAKUSHO KK) 7 June 1988 see abstract ---	3,7, 10-12, 23,24
A	EP,A,0 492 326 (BOEHRINGER MANNHEIM GMBH) 1 July 1992 see column 6, line 31 - line 54; figures 2,4 ----	11,12, 14,15
A	EP,A,0 165 535 (MILES LABORATORIES, INC) 27 December 1985 see page 17, line 28 - page 19, line 14 ----	6,18
A	FR,A,2 615 953 (CENTRE TECHNIQUE DE L'INDUSTRIE DE PAPIERS CARTONS ET CELLULOSES) 2 December 1988 see page 2, line 31 - page 3, line 23 ----	3,4
A	EP,A,0 560 411 (UNILEVER N.V.) 15 September 1993 see page 11, line 1 - page 15, line 5 see figures 1-14 & EP,A,0 291 194 cited in the application -----	7,11,23

between the individual consumer and the medical profession (GP).

5 There are many assays indicative of physiological changes in the human body which currently can only be performed using sophisticated laboratory techniques. In order to provide useful information concerning the individual under test, such assays generally need to yield a result in precise numerical terms, eg. the concentration of a specific analyte in a body fluid.

10 Accordingly there is a need for an assay system, especially applicable to the testing of body fluid samples in the home, which combines convenience of sample testing together with simple and cost-effective numerical determination of the assay result.

15 Many assay devices are described in the technical literature with suggestions that the assay result can be read using optical equipment. The use of fluorescence emission, or light reflectance, is often suggested. Such techniques are mostly appropriate for use in sophisticated laboratories. In EP-A2-212599, which describes multizone analytical elements having a detectable signal concentrating zone, the suggestion is made that a detectable signal indicative of an assay result in the zone can be measured by electromagnetic radiation, such as light, transmitted through the zone. EP-A2-212599 indicates that the element can be made from porous fibrous materials, such as paper and nitrocellulose. However, no practical details are provided to indicate how an accurate measurement might be made using transmitted light.

20 By the invention, we have found that quantitative information can be derived by transmission reading of an assay strip or the like if the incident electromagnetic radiation is uniform across a region of the test strip

## INTERNATIONAL SEARCH REPORT

Inter. nal Application No

PCT/EP 94/03700

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 G01N21/86 G01N33/558 G01N33/543

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 G01N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	DATABASE WPI Week 8503, Derwent Publications Ltd., London, GB; AN 85-016668 & JP,A,59 214 768 (MOCHIDA PHARM KK) 4 December 1984 see abstract	24,25,27
A	---	5,8-10, 17,21,23
A	EP,A,0 283 285 (DIAGNOSTIC SYSTEMS, INC.) 21 September 1988 see column 6, line 28 - column 8, line 34; figures 1-10 ---	3,7,11, 13,23,24
	--- -/--	

☒ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

## \* Special categories of cited documents :

- \* "A" document defining the general state of the art which is not considered to be of particular relevance
- \* "E" earlier document but published on or after the international filing date
- \* "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \* "O" document referring to an oral disclosure, use, exhibition or other means
- \* "P" document published prior to the international filing date but later than the priority date claimed

- \* "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \* "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \* "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- \* "&" document member of the same patent family

Date of the actual completion of the international search

26 January 1995

Date of mailing of the international search report

17.02.95

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

De Kok, A



which encompasses and extends beyond the test zone.

5 In one embodiment, the invention provides a method of "reading" the result of an assay effected by concentrating a detectable material in a comparatively small zone of a carrier in the form of a strip, sheet or layer through the thickness of which electromagnetic radiation, such as light, is transmissible, wherein at least a portion of one face of said carrier is exposed to incident electromagnetic radiation which is substantially uniform across the entire portion, said portion including said zone, and electromagnetic radiation emerging from the opposite face of said carrier is measured to determine said assay result.


10  
15 Preferably, the incident electromagnetic radiation is of substantially uniform intensity.

20 This uniformity can be achieved, for example, by providing a colimated source of electromagnetic radiation, using conventional focussing means such as lenses and light guides to provide parallel incident electromagnetic radiation which falls essentially normally across the entire exposed portion of the carrier.

25 However, in a more preferred embodiment of the invention, the incident electromagnetic radiation is diffuse and bathes the exposed portion of the carrier uniformly in a randomly scattered manner.

30 In another embodiment, the invention provides an assay device comprising a porous liquid-permeable carrier strip or sheet through the thickness of which electromagnetic radiation is transmissible diffusely, said carrier being within a casing, said carrier including at least one detection zone in which an assay result is revealed by specific binding of a detectable material directly or indirectly to a binding agent immobilised in said detection

35

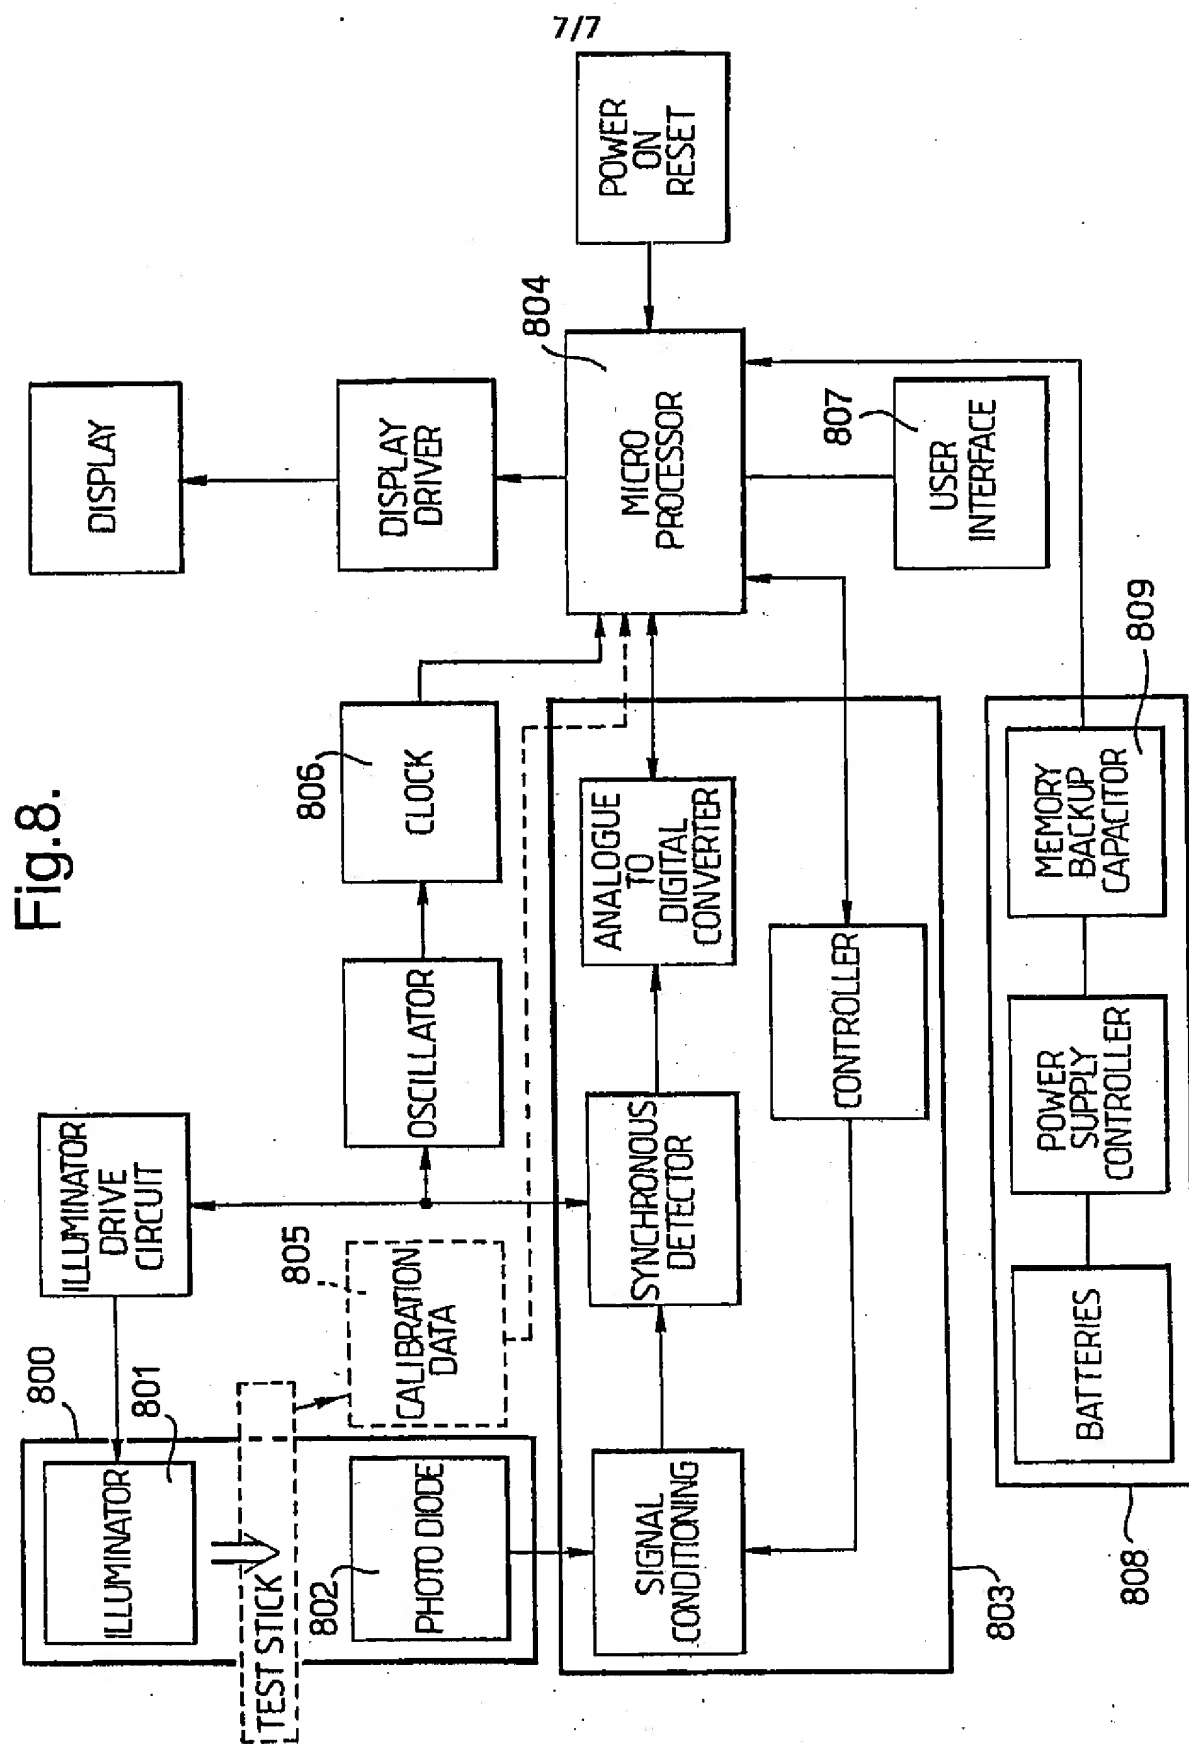

5 zone, detection of said material being effected as a response to said electromagnetic radiation, and said casing having electromagnetic radiation transmitting regions enabling electromagnetic energy from an external source to be passed through said device, said detection zone lying in the electromagnetic radiation path between said electromagnetic radiation transmitting regions.

10 Preferably, the porous carrier strip or sheet comprises paper, nitrocellulose or the like, preferably of a thickness not exceeding 1mm.

15 In yet another embodiment, the invention provides an assay device and assay result reader combination, wherein:

20 a) said device comprises a porous liquid-permeable carrier strip or sheet through the thickness of which electromagnetic radiation is transmissible diffusely, said carrier preferably being within a casing or cover, said carrier including at least one detection zone in which an assay result is revealed by specific binding of a detectable material directly or indirectly to a binding agent immobilised in said detection zone;

25 b) said casing or cover, if present, has electromagnetic radiation transmitting regions enabling electromagnetic radiation from an external source to be passed through said device, said detection zone lying in a path between said transmitting regions;

30 c) said assay result reader has receiving means for receiving at least a portion of said device, said portion including said detection zone to present said detection zone to reading means, said reading means incorporating a source of uniform electromagnetic radiation and one or more sensors located such that upon insertion of said device into said receiving means, electromagnetic radiation can be

35

6/7

Fig.5.

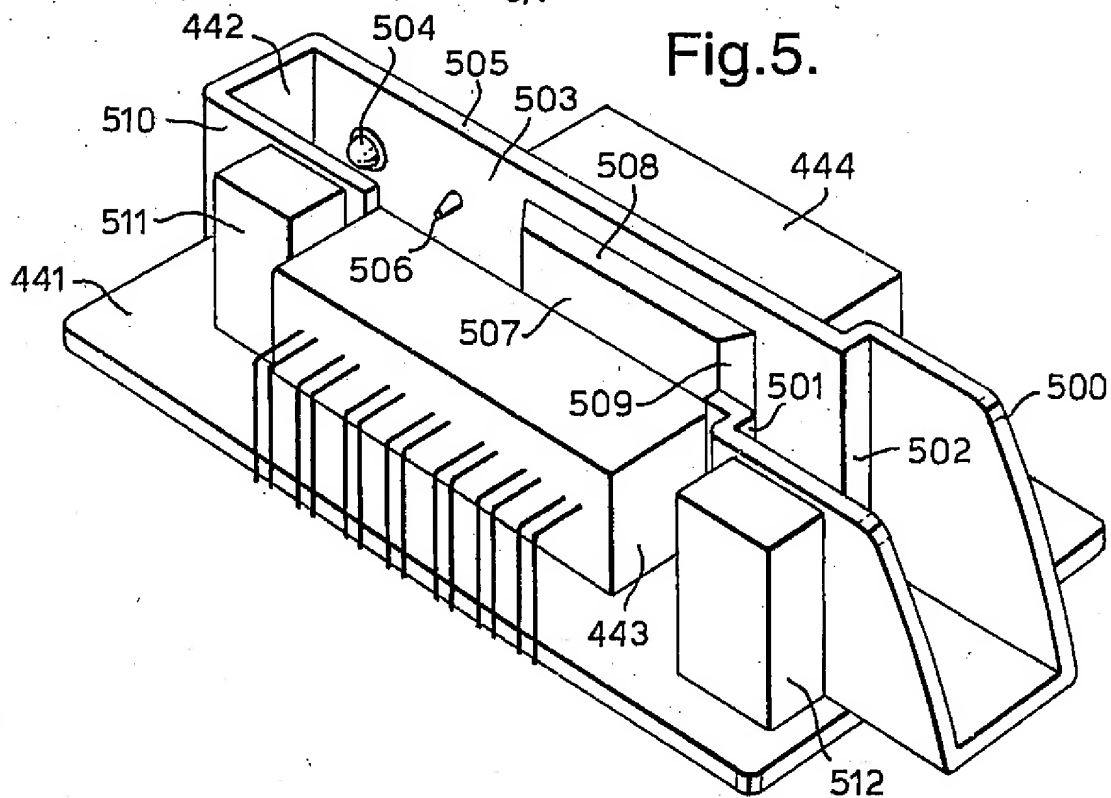


Fig.6.


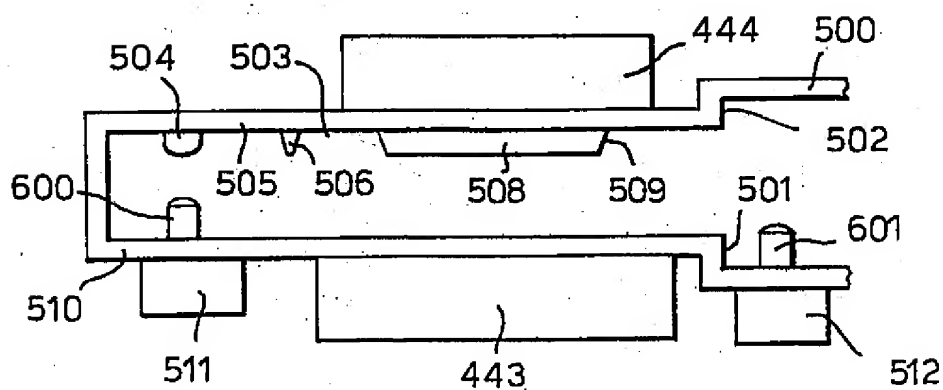


Fig.7.

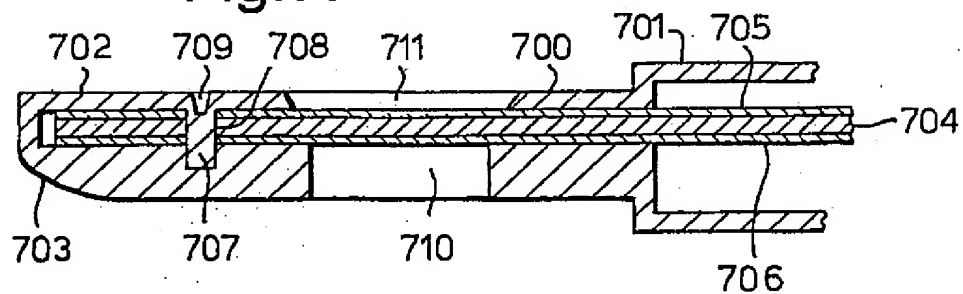

passed through said device and the intensity of electromagnetic radiation emerging from said device can be detected by said sensor(s).


5 Preferably, said receiving means incorporates interlocking means engagable with corresponding interlocking means on said device to ensure that upon receipt of said device by said reader said detection zone(s) is located and maintained in a predetermined spacial relationship relative  
10 to said reading means.

Preferably, said receiving means includes actuating means triggered by said receipt of said device, said actuating means causing said reading of said detection zone(s) to be  
15 initiated.

If the assay device is provided with a casing, it is advantageous if said device casing includes internal registration means which engages with corresponding  
20 registration means associated with said carrier such that said detection zone within said device casing is located in a predetermined spacial relationship relative to said registration means on said device casing. Preferably, said internal registration means comprises a pin or the like,  
25 engagable with a hole, indentation of the like in said carrier, said detection zone being at a predetermined location on said carrier relative to said hole or indentation.

30 During manufacture of said assay device, said corresponding registration means may be used to facilitate or control accurate formation, e.g. by means of reagent printing techniques, of said detection zone on said carrier. In addition, or alternatively, accurate placement of said  
35 carrier within said device casing can be facilitated or controlled by said registration.

Fig.4c.

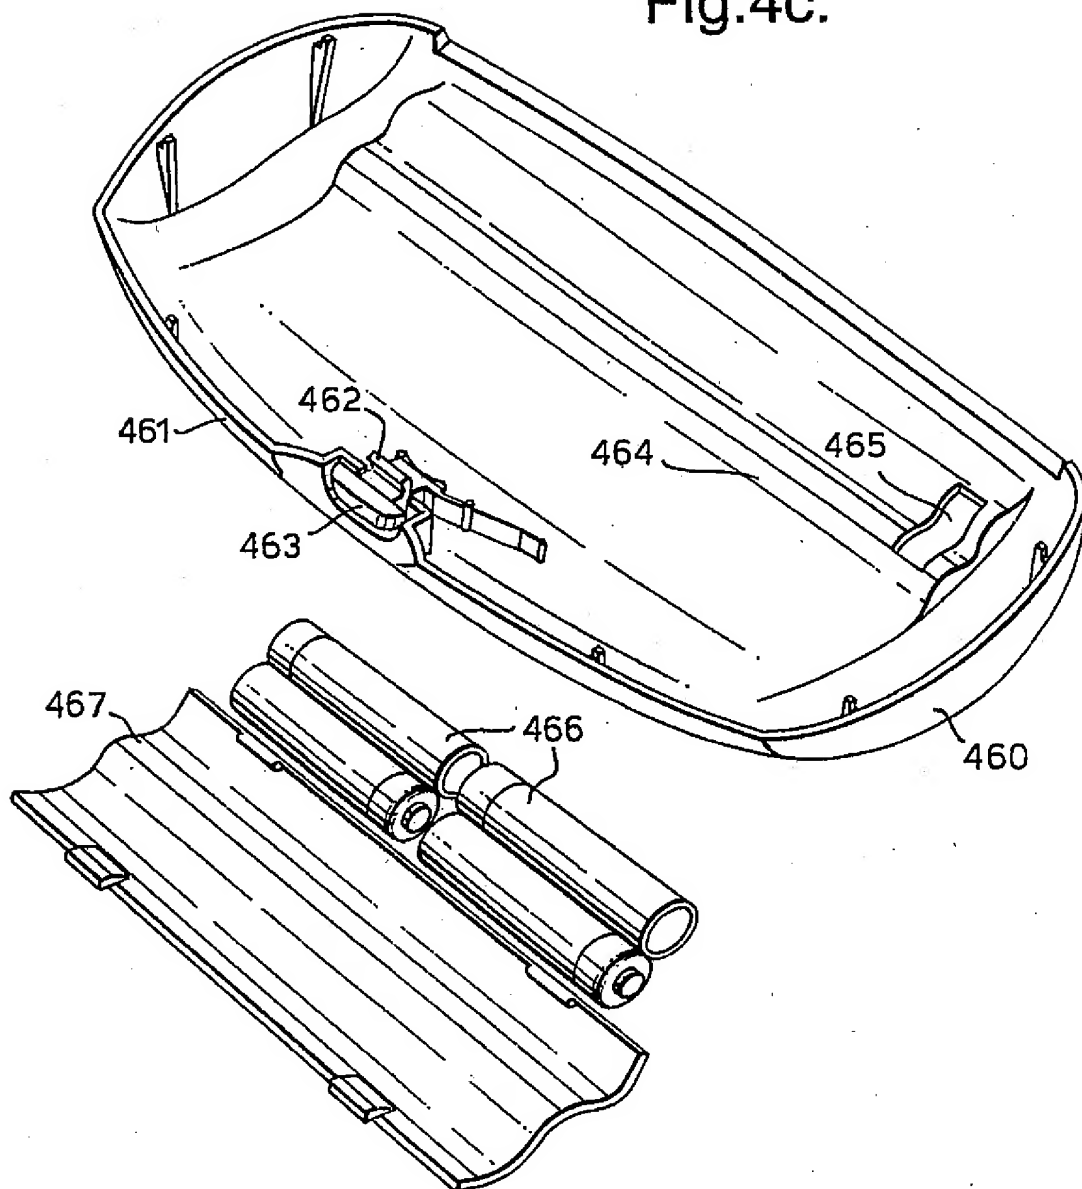

5 In a further embodiment, the invention provides an assay result reader, for use in conjunction with an assay device comprising a porous liquid-permeable carrier strip or sheet through the thickness of which electromagnetic radiation is transmissible, said carrier including a detection zone in which an assay result is revealed by specific binding of a detectable material directly or indirectly to a binding agent immobilised in said detection zone, detection of said material being effected as a response to said  
10 electromagnetic radiation, said assay result reader comprising:

15 a) receiving means for receiving at least a portion of said assay device, said portion including said detection zone;

b) reading means associated with said receiving means, said reading means comprising:


20 i) at least one source of uniform diffuse (preferably electromagnetic radiation; and  
ii) one or more sensors capable of detecting the intensity of said electromagnetic radiation;

25 said source and said sensor(s) being positioned such that when said portion of said assay device is received within said receiving means, said detection zone is disposed in a path between said source and said sensor(s).

30 The assay device/reader combination can be supplied to the consumer as a single test kit. In general however, whereas the reader will be a relatively permanent unit which the consumer can use time and again (and which may be provided with an electronic memory/data-processing facility which  
35 enables the results of many sequential assays to be evaluated) the testing devices will be intended for use only once and thereafter will be discarded. Accordingly,

4/7

Fig. 4b.

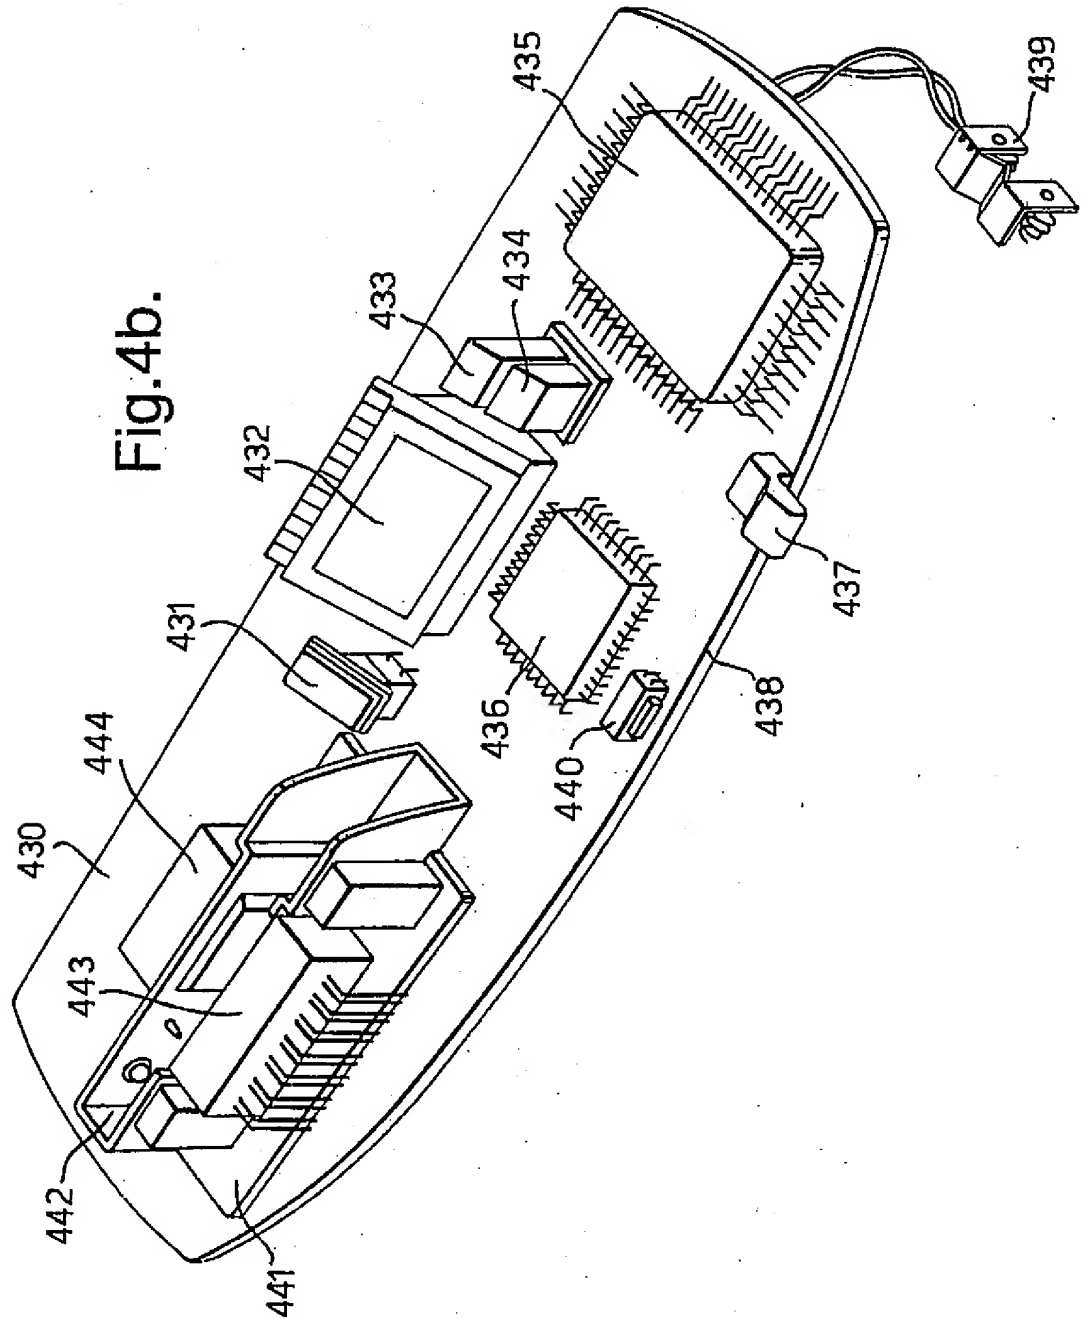



the test devices may be supplied to the consumer separately from the reader, e.g. in multi-packs.


5 By ensuring precise interlocking between the testing device and the reader, and also ensuring precise registration of the location of the detection zone within the testing device itself, the testing zone will be presented to the reader in a constant pre-determined position every time a testing device is inserted into the reader. The construction of the optical system within the reader (light source and sensors) can therefore be kept as simple as possible, because it is not essential for the sensors to include any scanning facility, for example, which would otherwise be required if the exact location of the detection zone was not known. By avoiding the need for a sophisticated optical reading system, the cost of the reader/monitor may be reduced. Simplification of the optical reading system may also enable the reader/monitor to be of small size which will assist convenient and unobtrusive use in the home. Of course, a scanning facility can be included in the reader if desired.

25 An additional benefit of providing an internal registration system which ensures precise location of the detection zone within the test device, is that automated manufacture and quality control of the testing devices can be facilitated. Because it is envisaged, for example, in the case of an ovulation cycle monitor, that the consumer will need to use several testing devices each month, the testing devices may need to be manufactured in large numbers at low cost. Internal registration can facilitate automated manufacture and high throughput.

35 In principle, any electromagnetic radiation can be used to effect the transmission measurement in the invention. The electromagnetic radiation should preferably be capable of being rendered diffuse. Preferably the electromagnetic

3/7

Fig.4 a.

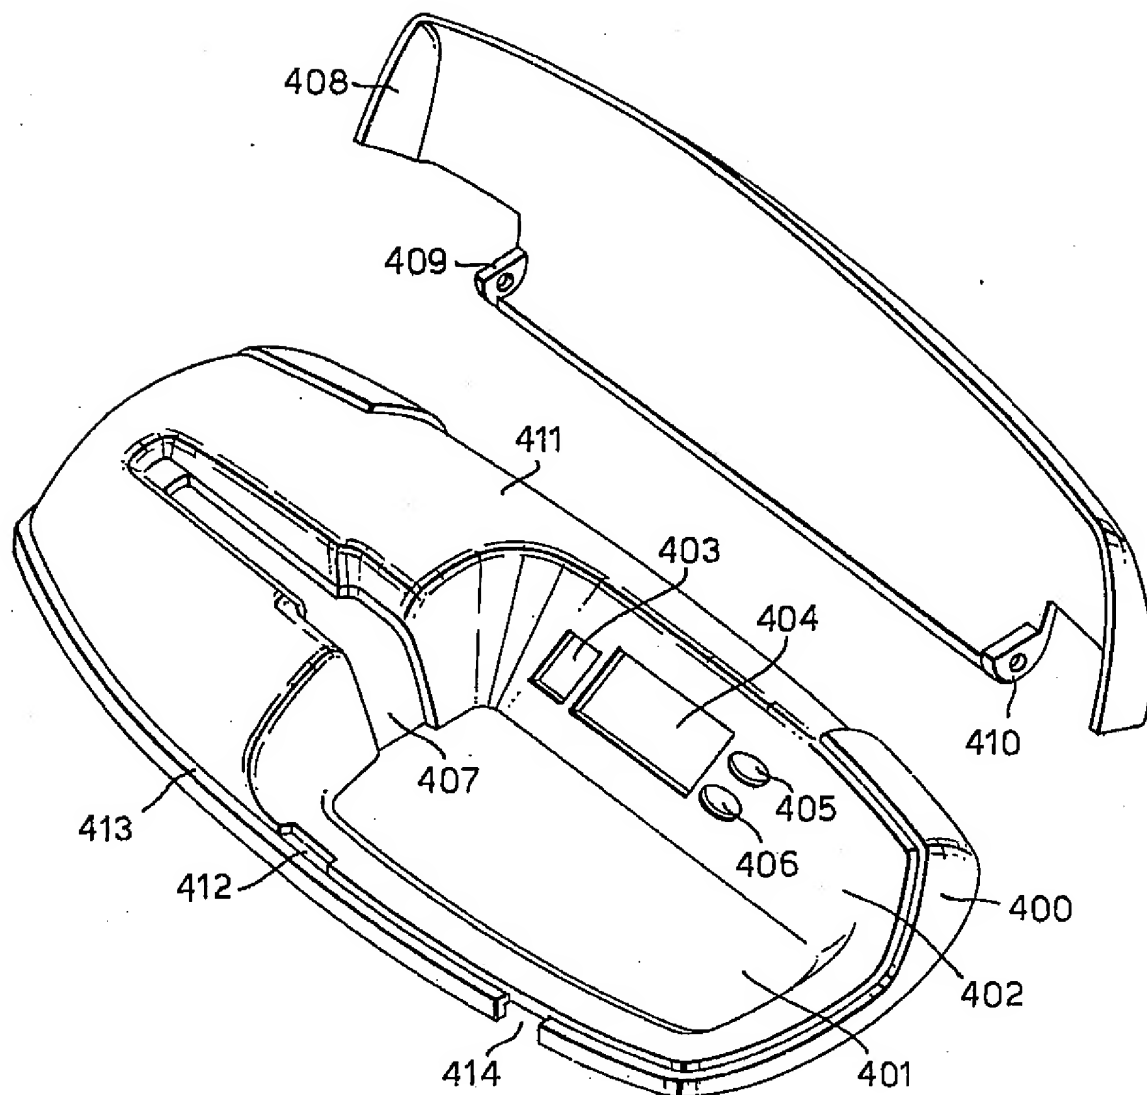


radiation is light in the visible or near-visible range. This includes infra-red light and ultra-violet light. It is generally envisaged that the detectable material used as a label in the assay is one which will interact with light in the visible or near visible range, eg. by absorption. The wavelength of the electromagnetic radiation chosen is preferably at or near a wavelength which is strongly influenced, eg. absorbed, by the label. For example, if the label is a substance which is strongly coloured, ie. visible to the naked human eye when the material is concentrated, the ideal electromagnetic radiation is light of a complementary wavelength. Particulate direct labels, for example, metallic (eg. gold) sols, non-metallic elemental (e.g. Selenium, carbon) sols, dye sols and coloured latex (polystyrene) particles are ideal examples. For instance, in the case of blue-dyed latex particles, the ideal electromagnetic radiation is visible red light which will be strongly absorbed by the blue particles.

In a preferred embodiment of the invention, the transmitted electromagnetic radiation reaching the sensor(s) should be diffuse. The diffuseness may arise as a consequence of transmission of the electromagnetic radiation through the carrier strip or sheet, but more preferably is contributed by the source of the electromagnetic radiation emitting the energy in a highly diffuse form. In a preferred embodiment of the invention the source produces highly diffuse radiation and the carrier strip or sheet through which this radiation subsequently is transmitted is in comparative terms a much weaker diffuser.

A primary advantage of the use of diffuse light or other radiation in the context of the invention is that the reading of the assay result is much less likely to be adversely influenced by blemishes or contaminating material on the assay device. For example, dirt or scratches on the assay device in the region through which the radiation must

**Fig. 3.**

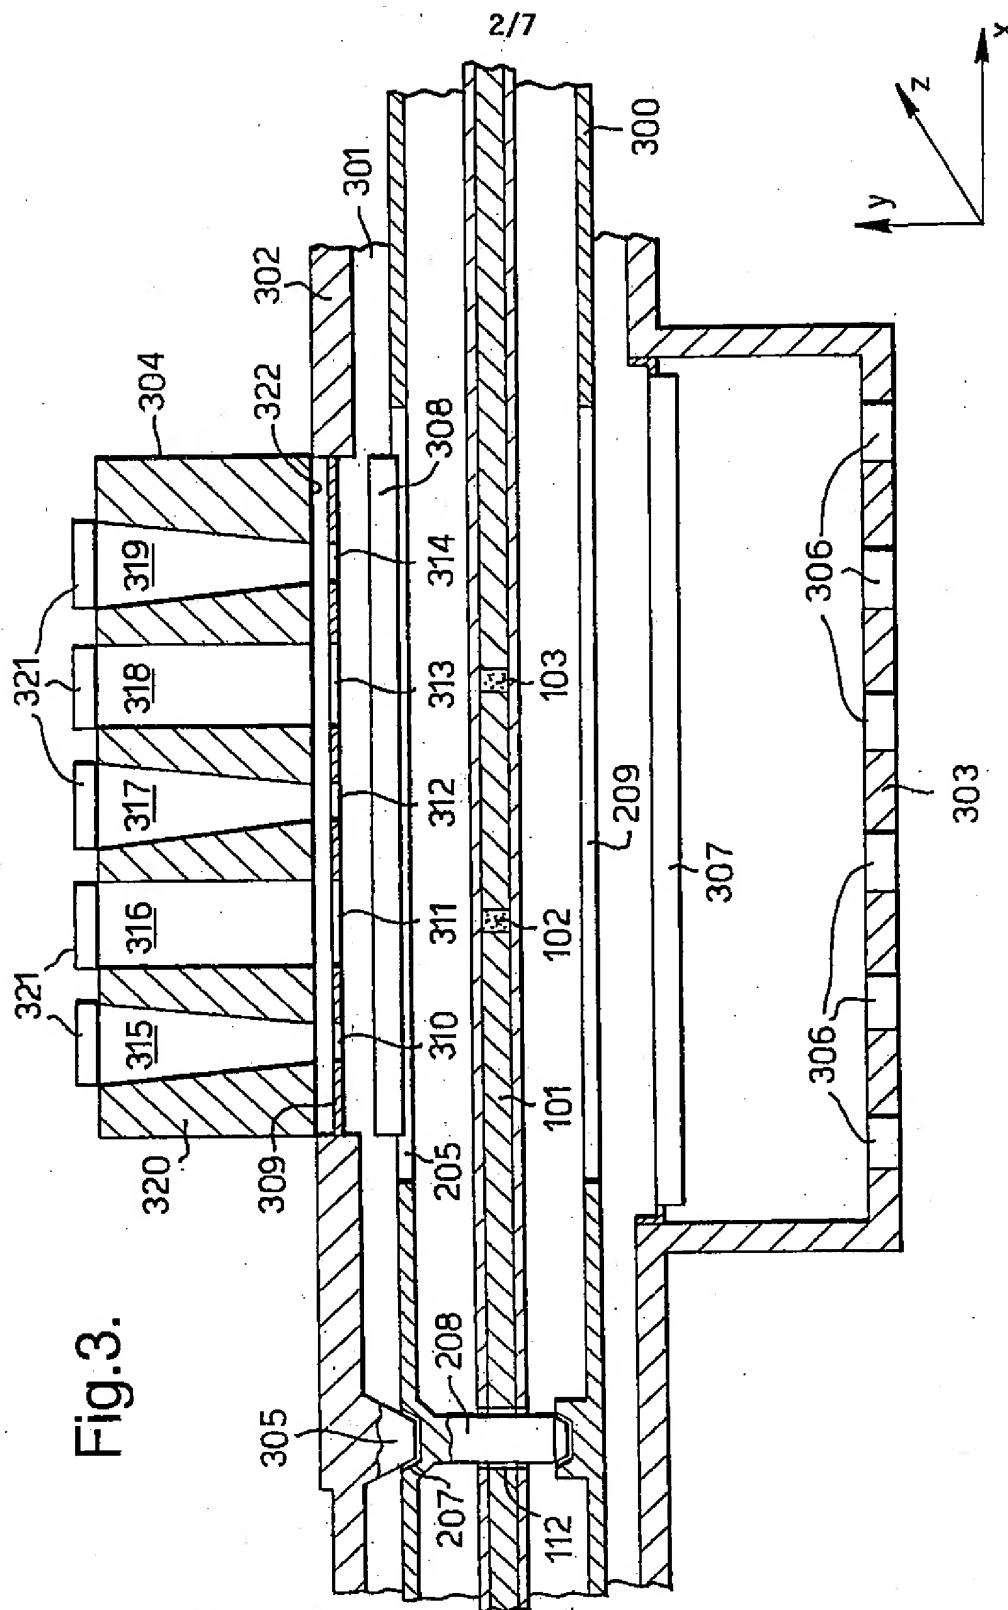

be transmitted could strongly interfere with the accuracy of the determined result if focussed rather than diffuse light is used. By the use of a diffuse light source in accordance with the invention, it is possible to provide an assay result reader which can accurately interpret the result of an assay conducted even in an essentially transparent assay device without the assay result being adversely affected by minor contamination or damage (eg. superficial scratches) to the assay device.

In a preferred embodiment of the invention, the electromagnetic radiation from the source is pulsed. By synchronising the detectors (sensors) so that they function only in phase with the pulsed radiation source, it is possible to eliminate any background interference that might be caused by external radiation, e.g. ambient light. It is envisaged that the assays will mostly be conducted under circumstances of natural daylight or, even more often, artificial light. Artificial light is usually of a pulsed nature (typically 50-100Hz) caused by the alternating nature of electricity supplies. By adopting a pulsed radiation source for the illumination of the assay device within the reader, the intrusion of natural daylight can be ignored. By selecting the pulse frequency such that it is sufficiently different from the prevailing artificial light, any interference due to artificial light can also be avoided. Preferably the pulse frequency of the energy should be at least about 1 kHz. An ideal pulse frequency is about 16 kHz. The electronics necessary to achieve synchronous pulsed sensing are familiar to those skilled in the art.

The use of pulsed light is very advantageous because it renders it unnecessary for the monitor to be "light tight". Not merely does this simplify the construction of the monitor but the reading of the assay result can be performed while the monitor is "open", thus simplifying the


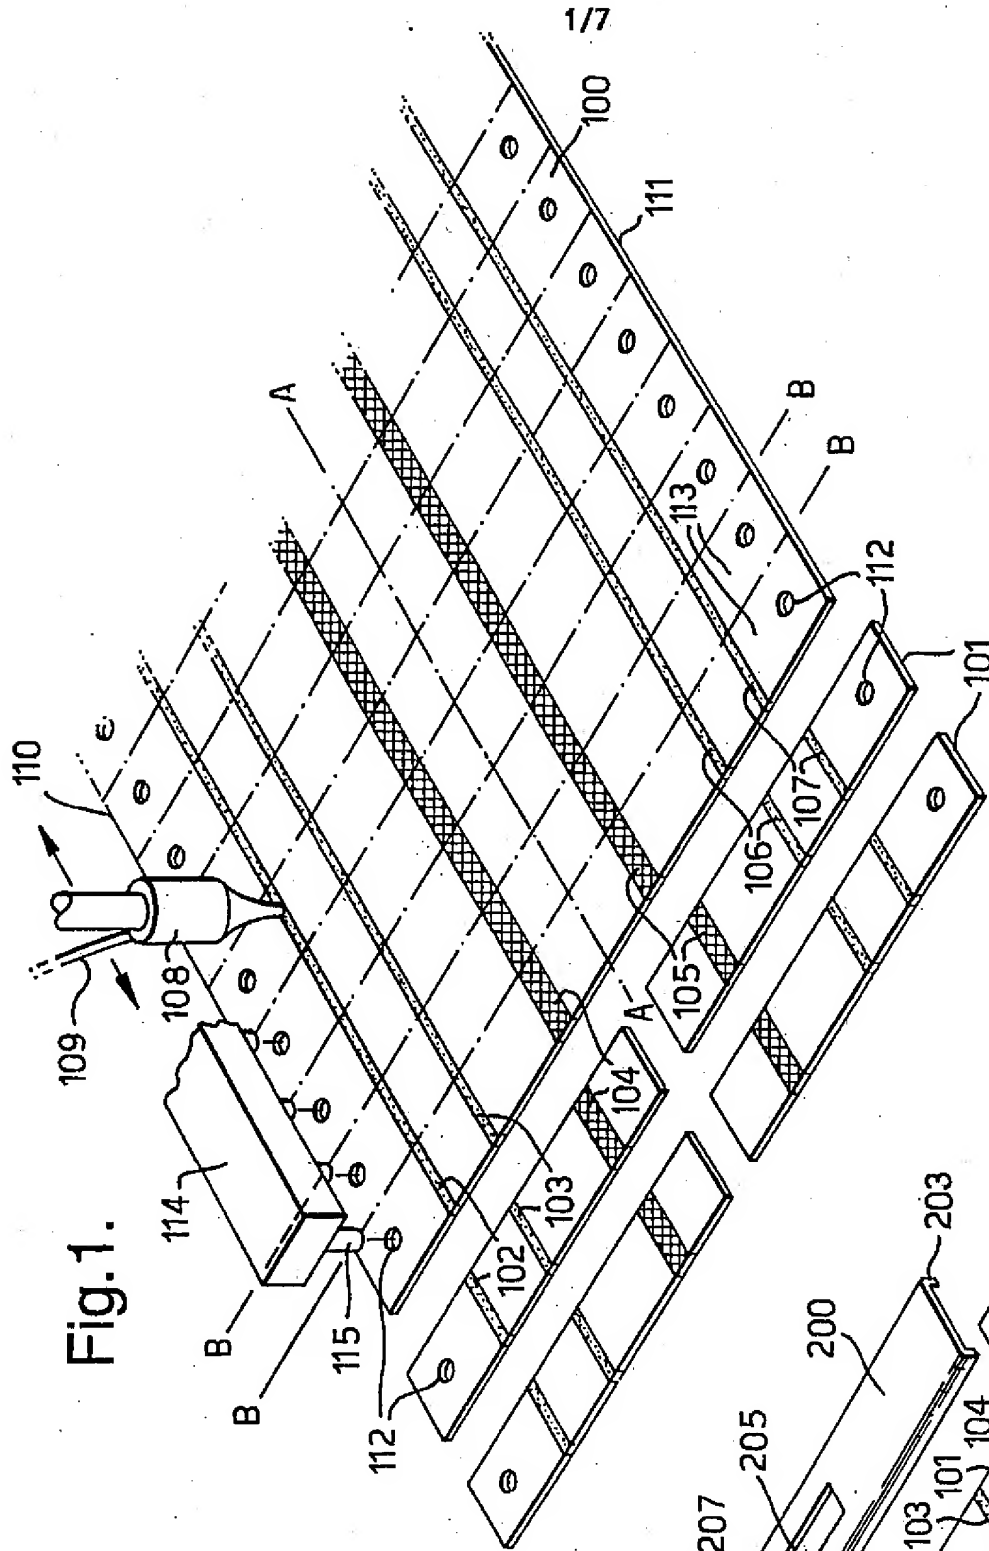


Fig. 1.

Fig. 2.

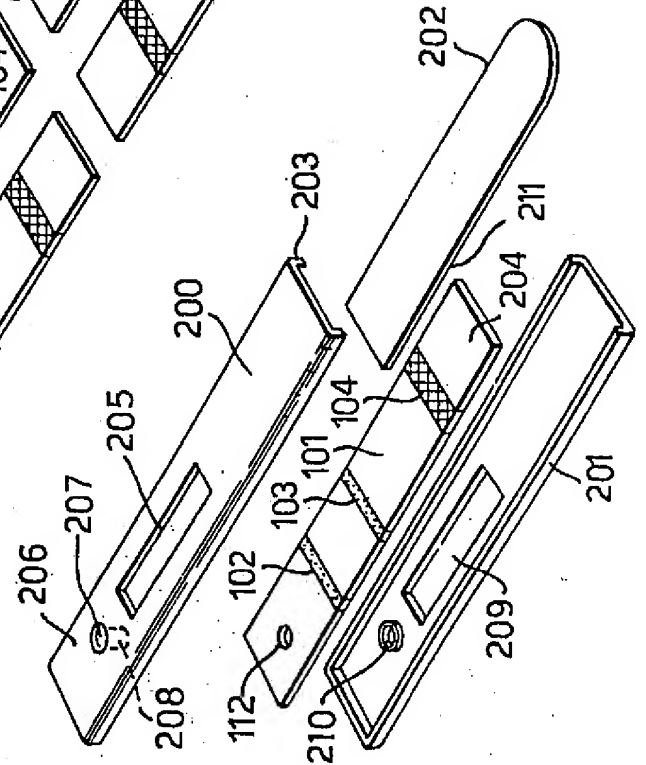

operation for the user.

5 The source of light or other electromagnetic radiation can  
comprise entirely conventional components. Ideal examples  
are commercially available LED's, preferably chosen to give  
a suitable wavelength of light that is strongly absorbed by  
the detectable material concentrated in the test zone(s).  
10 Light from the LED's should be passed through a strong  
diffuser before reaching the assay device. If desired, an  
array of LED's which are energised in turn can be used.

15 Suitable diffusers can be made, for example, from plastics  
materials, and are available commercially. If necessary,  
the light-scattering properties of the diffusing material  
can be enhanced by including particulate materials such as  
Titanium dioxide and Barium sulphate. An ideal diffusing  
material comprises polyester or polycarbonate, containing  
Titanium dioxide. A good inclusion level for the  
20 particulate material is at least about 1% by weight,  
preferably about 2%. By the use of a diffuser, all  
relevant regions of an assay strip may be measured  
simultaneously, and differences in light output from the  
source are eliminated.

25 The sensor(s) to detect emergent light can be conventional  
components such as photodiodes, e.g. silicon photodiodes.

30 Preferably, a second diffuser, which can be made from the  
same material as the primary diffuser, is located in front  
of the sensor(s). This ensures that the view seen by the  
sensor is not affected by the presence or absence of a  
test strip in the reading head. In consequence, the  
monitor can be calibrated in the absence of a test strip,  
and then measure an assay result in the presence of an  
35 assay strip.

By employing a uniform light source in accordance with the

reader combination according to any one of claims 11 to 21, the assay device being one of a plurality of identical such devices provided as part of the kit.

- 5        23. A method of determining the concentration of an analyte, in a sample liquid involving use of an assay device and assay result reader combination according to any one of claims 11 to 21.
- 10       24. A method of "reading" the result of an assay effected by concentrating a detectable material in a comparatively small zone of a carrier in the form of a strip, sheet or layer through the thickness of which electromagnetic radiation is transmissible, wherein at least a portion of
- 15       one face of said carrier is exposed to incident electromagnetic radiation which is substantially uniform across the entire portion, said portion including said zone, and electromagnetic radiation emerging from the opposite face of said carrier is measured to determine said
- 20       assay result.
- 25       25. A method according to claim 24, wherein said incident electromagnetic radiation is of substantially uniform intensity across said exposed portion of said carrier.
26. A method according to claim 24 or claim 25, wherein said incident electromagnetic radiation is diffuse.
- 30       27. A method according to any one of the preceding claims, wherein said electromagnetic radiation is light preferably visible light.
- 35       28. A method according to any one of the preceding claims, wherein said detectable material is a particulate direct label.



invention, it is possible to provide a reading system for test strips and the like which is relatively tolerant to variation in the placement of the test zone(s) from one strip to another, in the absence of a scanning sensor. Further benefits are obtained if test zone placement is controlled, as described herein.

For the purposes of enhancing the likelihood of conception, assay devices have already been marketed which enable the user to monitor the urinary concentration of lutenizing hormone (LH) which peaks sharply approximately one day in advance of ovulation. Daily testing of urinary LH concentration is conducted, for example using "dipstick" technology with the assay result being provided by a coloured end point, the intensity of the colour being proportional to LH concentration. By providing the consumer with a colour chart which enables the daily result to be compared against a standard, the "LH surge" can be detected simply by eye. Unfortunately, the monitoring of LH concentration is a very rare example of an assay relying on semi-quantitative data which is amenable to such simple technology, being possible only because in relative concentration terms the LH surge is such a dramatic event. For most other potentially useful assays the analyte concentration changes in body fluids are much more subtle and only detectable accurately by instrumental means.

A need therefore exists to extend the currently available qualitative home-use testing technology into the area of precise quantitative testing. A convenient example, which is a logical extension of the present consumer interest in home-use pregnancy testing and ovulation prediction testing, is the extension into accurate monitoring of the ovulation cycle, not merely to enhance the likelihood of conception but indeed to provide reliable information for the purposes of contraception. Proposals have been made to analyse body fluids with this objective in mind. A common

corresponding registration means associated with said carrier such that said detection zone within said device casing or cover is located in a predetermined spacial relationship relative to said interlocking means on said device casing or cover.

15. Combination according to claim 14, wherein said internal registration means comprises a pin or the like, engagable with a hole or indentation in said carrier, said detection zone being at a predetermined location on said carrier relative to said hole or indentation.

16. Combination as claimed in any one of claims 11 to 15, wherein said electromagnetic radiation from said source is diffuse.

17. Combination as claimed in any one of claims 11 to 16, wherein said electromagnetic radiation is light.

18. Combination as claimed in any one of claims 11 to 17, wherein said electromagnetic radiation from said source is pulsed.

19. Combination as claimed in any one of claims 11 to 18, wherein said carrier strip or sheet comprises paper, nitrocellulose or the like, preferably having a thickness not exceeding 1mm.

20. Combination as claimed in any one of claims 11 to 19, wherein said detectable material comprises a particulate direct label.

21. Combination as claimed in claim 11, wherein said electromagnetic radiation is visible light of a wavelength that is strongly absorbed by said particulate direct label.

22. A test kit comprising an assay device and assay result

theme is to monitor periodic fluctuations in various hormone metabolite levels in urine.

5 The invention can be used in the determination of any body fluid analyte, especially in the monitoring of the human ovulation cycle by the determination of one or more hormones or metabolites thereof in body fluid, such as urine, for example either LH and/or estrone-3-glucuronide (E3G).

10 Within the preferred context of the present invention it is envisaged that a home-use sample liquid testing device will include a porous carrier material, such as a strip, through which applied sample liquid such as urine can permeate and  
15 wherein the assay result occurs by means of specific binding of a detectable material in a precisely-defined region (detection zone) of the carrier, such as a narrow line or small dot, containing an immobilized specific binding reagent. The invention is therefore concerned with  
20 ways in which localisation of a detectable material in such a detection zone can be determined accurately in a simple and cost-effective manner. Home-use devices for the analysis of urine, for example in pregnancy tests and ovulation prediction tests, are now widely available  
25 commercially. Many such devices are based on the principles of immunochromatography, and typically comprise a hollow casing constructed of plastics material containing a porous assay strip carrying pre-dosed reagents. The reagents within the device may include one or more reagents  
30 labelled with a direct label, such as a dye sol, a metallic (e.g. gold) sol, or a coloured latex (e.g. polystyrene) microparticle, which are visible to the eye when concentrated in a comparatively small test area of the strip. The user merely needs to apply a urine sample to  
35 one part of the casing to initiate the assay. The assay result becomes visible by eye within a few minutes without further action by the user. Examples of such devices are

detectable material directly or indirectly to a binding agent immobilised in said detection zone;

5       b)    said casing or cover (if present) has electromagnetic energy transmitting regions enabling electromagnetic radiation from an external source to be passed through said device, said detection zone lying in the path between said transmitting regions;

10       c)    said assay result reader includes receiving means for receiving at least a portion of said device, said portion including said at least one detection zone, to present said at least one detection zone to reading means, said reading means incorporating a source of uniform electromagnetic radiation and one or more sensors located such that upon  
15       insertion of said device into said receiving means, electromagnetic radiation can be passed through said device and the intensity of electromagnetic radiation emerging from said device can be detected by said sensor(s).

20       12.    Combination as claimed in claim 11, wherein said receiving means incorporates interlocking means engagable with corresponding interlocking means on said device to ensure that upon receipt of said device by said reader said  
25       detection zone(s) is located and maintained in a predetermined spacial relationship relative to said reading means.

30       13.    Combination as claimed in claim 11 or claim 12, wherein said receiving means includes actuating means triggered by said receipt of said device, said actuating means causing said reading of said detection zone(s) to be initiated.

35       14.    Combination as claimed in any one of claims 11 to 13, wherein said device has a casing or cover which includes internal registration means which engages with

described in EP-A-291194 and EP-A-383619, the disclosures of which are incorporated herein by reference. Sample collection is conveniently achieved by means of a bibulous member which forms part of the device and which can readily  
5 take up sample liquid, e.g. from a urine stream. Optionally the bibulous member can protrude from the casing of the device to facilitate sample application.

Other embodiments of the invention, which will be apparent  
10 from the following detailed description, include assay devices for use as part of the reader/assay device combination, methods of manufacturing such assay devices, and methods of use of such assay devices and readers.

15 By way of example only, assay devices and readers in accordance with the invention will now be described with reference to the accompanying drawings, of which:

20 Figure 1 shows a general view of a sheet of porous material, e.g. paper, during the course of reagent deposition on the sheet and sub-division of the sheet into assay strips.

25 Figure 2 shows an "exploded" view of an assay device of the invention incorporating an assay strip made as shown in Figure 1.

30 Figure 3 shows in diagrammatic cross-section an assay device of Figure 2 located within the reading head of a monitor in accordance with the invention, working by light transmission through the assay strip. The y axis is distorted to show the arrangement of components.

35 Figures 4a, 4b and 4c show in partially "exploded" form the main features of a complete monitor in accordance with the invention, namely:

carrier strip or sheet through the thickness of which electromagnetic radiation is transmissible diffusely, said carrier being within a casing, said carrier including at least one detection zone in which an assay result is revealed by specific binding of a detectable material directly or indirectly to a binding agent immobilised in said detection zone, detection of said material being effected as a response to said electromagnetic radiation, and said casing having electromagnetic radiation transmitting regions enabling electromagnetic radiation from an external source to be passed through said device, said detection zone lying in the electromagnetic radiation path between said electromagnetic energy transmitting regions.

15

8. An assay device according to claim 7, wherein said electromagnetic radiation comprises light, preferably visible light.

20

9. An assay device according to claim 7 or claim 8, wherein said detectable material is a particulate direct label.

25

10. An assay device according to any one of claims 7 to 9, wherein said carrier strip or sheet comprises paper, nitrocellulose or the like, preferably having a thickness not exceeding 1mm.

30

11. An assay device and assay result reader combination, wherein:

35

a) said device comprises a porous liquid-permeable carrier strip or sheet through the thickness of which electromagnetic radiation is transmissible diffusely, said carrier preferably being within a casing or cover, said carrier including at least one detection zone in which an assay result is revealed by specific binding of a

Figure 4a: the lid and upper half of the casing;

Figure 4b: an electronic circuit board incorporating a reading head;

5

Figure 4c: the lower half of the casing and associated battery container.

10

Figure 5 shows the reading head seen in Figure 4b on an enlarged scale.

Figure 6 shows a view directly downwards into the test device receiving slot of the reading head of Figure 5.

15

Figure 7 is a cross-section of one end of a test device designed for insertion into the receiving slot of the reading head.

20

Figure 8 shows, in schematic form, the basic functions that may be required in an electronic monitor for use in accordance with the invention, as applied to the human ovulation cycle.

25

Referring to Figure 1, the sheet 100 of porous material, e.g. nitrocellulose, is intended to be divided into a plurality of identical assay strips 101 by cutting along central axis A-A and the lateral axes B-B.

30

Parallel lines (102-107) of assay reagents are placed on sheet 100 prior to sub-division. For the purposes of example only, the reagents are assumed to be a first immobilised antibody in lines 102 and 107, and a second different immobilised antibody in lines 103 and 106. Reagent deposition can be by means of a "pen" 108 or the like operated on a computer-controlled "x-y" plotting mechanism (not shown) and fed with appropriate buffered reagent solution via a metered flexible tube 109. If the

35

directly or indirectly to a binding agent immobilised in said detection zone, detection of said material being effected as a response to said electromagnetic radiation, said assay result reader comprising:

5

a) receiving means for receiving at least a portion of said assay device, said portion including said detection zone;

10

b) reading means associated with said receiving means, said reading means comprising:

i) at least one source of diffuse electromagnetic radiation; and

15

ii) one or more sensors capable of detecting the intensity of said electromagnetic radiation;

said source and said sensor(s) being positioned such that when said portion of said assay device is received within said receiving means, said detection zone is disposed in the path between said source and said sensor(s).

20

4. An assay result reader according to claim 3, having a diffuser in front of said one or more sensors such that electromagnetic radiation from said diffuse source must pass through said diffuser before reaching said one or more sensors, and said detection zone of said assay device being disposed in the path between said diffuse source and said diffuser.

25

30

5. An assay result reader according to claim 3 or claim 4, wherein said electromagnetic radiation is light.

35

6. An assay result reader according to claim 5, wherein said light is pulsed, preferably having a pulse frequency of at least about 1 kHz.

7. An assay device comprising a porous liquid-permeable



material of sheet 100 is nitrocellulose, reagents such as antibodies and antigens can be immobilised by simple direct application onto the nitrocellulose, followed by blocking of the sheet material, for example with albumen or polyvinyl alcohol. Following reagent deposition and blocking, two lines 104 and 105 of mobile labelled reagent, such as antigen (e.g. E3G) or another antibody (e.g. anti-LH) labelled for example with a particulate direct label such as coloured latex, can be deposited. This deposition can be for example by means of another pen (not shown). Alternatively, the labelled reagent(s) can be held in a separate porous pad or the like, rather than being applied directly to the test strip material.

In order to achieve precise location of the reagent-containing lines, each longitudinal periphery 110, 111 of sheet 100 is pierced with a plurality of identical small holes 112 each one being situated within the width of a designated strip 113. Holes 112 are made in sheet 100 prior to the deposition of any reagents. The untreated sheet is located on a frame (not shown) or similar operating surface by means of a bar 114 pressed downwardly onto each lateral periphery of the sheet. Only one of these bars is (partially) shown. Each bar has a plurality of downwardly projecting pins 115, each of which locates precisely into one of the holes 112. The tracking of the reagent-depositing pen 108 is registered precisely with the position of the bars holding the sheet, and accordingly the reagent deposition is made in a predetermined precise line relative to the perforations in the sheet.

Following all necessary reagent depositions and other treatments of the sheet, the sheet is subdivided by cutting means (not shown) into individual identical strips 101. Each individual strip therefore contains one locating hole 112 with two reagent-containing lines or reaction zones (e.g. 102 and 103) located relative to hole 112 in precise

CLAIMS

- 5        1.    An assay result measuring device for reading the result of an assay effected by concentrating a detectable material in a small zone of a porous sheet or strip, which device comprises:
- 10        a)    a source of diffuse light having a wavelength that is strongly absorbed by said detectable material;
- 15        b)    sensing means to sense incident light from said source;
- 20        c)    means for holding said porous sheet or strip with said small zone in a light path between said source and said sensor; and
- 25        d)    electronic means connected to said sensing means, said electronic means being programmed to derive from sensed incident light a measure of the extent to which said detectable material has become concentrated in said small zone.
- 30        2.    A device according to claim 1, wherein said diffuse light is pulsed, and said electronic means is programmed to control said sensing means such that said sensing means only senses incident light in phase with said pulsed light, said light preferably having a pulse frequency of at least about 1 kHz.
- 35        3.    An assay result reader, for use in conjunction with an assay device comprising a porous liquid-permeable carrier strip or sheet through the thickness of which electromagnetic radiation is transmissible, said carrier including a detection zone in which an assay result is revealed by specific binding of a detectable material

predetermined positions extending across the width of each strip. At a location remote from hole 112 is a region (e.g. 104) of the strip bearing the mobile labelled reagent. The exact position of the labelled reagent relative to the hole is not necessarily as critical as the location of the reaction zones.

By way of example only, the individual strips will typically have a length of about 40mm to about 80mm, and a width of about 5mm to about 10mm, as is already conventional in the assay device art. A reagent-containing detection zone such as the reaction zones 102 and 103, will typically be a line of width about 1mm running laterally across the strip. A small dot, e.g. circular with diameter of about 1mm to about 3mm, is an alternative. The detection zone is therefore only a relatively small proportion of the total area of the strip. If appropriate for the purposes of the assay, multiple detection zones containing the same or different reagents can be placed on each strip. This may necessitate more than one labelled component being used; multiple mobile labelled components can be placed upstream on the strip or elsewhere within the device (eg. in a sample application pad or wick, as described below).

Referring to Figure 2, an assay device of the invention comprises a plastics casing having upper and lower halves 200 and 201 adapted to contain the assay strip 101 and also a bibulous sample receiving member 202 which can extend out of one end 203 of the assembled casing. In the assembled device the bibulous receiving member 202 overlaps the end 204 of the assay strip adjacent to the deposited labelled reagent. The upper half 200 of the casing includes a window or aperture 205 through which both detection zones 102 and 103 can be observed from outside the casing. Upper half of the casing contains on its external surface 206 a circular depression 207 on the central longitudinal access

constructed as hereinbefore described with reference to Figures 3 to 8.

5 The intensities of the two test lines respectively represented the concentrations of LH and E3G in a urine sample applied to the testing device.

10 The testing device was inserted and removed from the monitor 10 times. The percentage light transmission for each reading was as follows:

	LH	E3G
	44.0	39.3
	43.8	39.3
15	43.8	39.5
	43.8	39.3
	43.8	39.3
	43.9	39.4
	43.8	39.2
20	43.9	39.2
	43.9	39.2
	43.9	39.4
	Mean:	43.9
		39.3
	sd:	0.1
25	cv%	0.2%
		0.3%

30 These results indicate that the reading system of the invention produces consistent data which is not affected significantly by any variability of test line placement when the test device is inserted in the monitor.

of the casing a short distance beyond the observation window relative to the end 203 of the casing accommodating the sample receiving member. On the inside of the upper half of the casing is a downwardly extending pin or peg 208 located directly below depression 207. The diameter of the downwardly extending pin or peg 208 matches that of the hole 112 in the assay strip 101, so that the strip can be positively located within the assembled device on the peg.

Lower half 201 of the casing also includes a light-transmitting window or aperture 209 which, in the assembled device, lies directly opposite to the result window 205 in the upper half of the casing. Lower half of the casing also contains a depression 210 which can accommodate the bottom end of the pin or peg 208 when the two halves of the casing are placed together to make an enclosure.

In the assembled device, the act of enclosing the strip and bibulous member between the upper and lower halves of the casing causes the overlapping portions 204 and 211 of the strip and bibulous member to be crimped together to provide a good moisture-conductive junction.

It is generally envisaged that the material of the casing will be opaque, e.g. white or coloured plastics material, but the casing can be translucent or indeed transparent if desired.

Referring to Figure 3, the assay device 300 is seen located within a slot 301 in a monitor 302. This region of the assay device includes the two opposing windows 205 and 209.

The casing of the monitor is slotted to receive the portion of the assay device incorporating the result windows. On opposing sides of the slot is a light source 303 and a reading head 304.

difficult to design a reflectance measurement system that minimises specular reflection to the extent possible with transmission measurement, especially using diffuse light as in accordance with the invention.

5 Reflectance systems require the use of a test surface that must be removed from the optical path for the purposes of calibration. This reference surface must not deteriorate if it is to form a part of the optical assembly. In  
10 addition, mechanical movement is required to displace such a reference material when an assay strip needs to be measured. Such problems are avoided by the invention.

In addition to the specific examples of detectable  
15 materials already mentioned herein, the invention can use as labels materials which block or reflect the electromagnetic radiation, rather than absorb it, e.g. "white" particles such as latex particles in their natural uncoloured state. Alternatively, the label can be a  
20 reactant or catalyst which participates in the generation of a radiation absorbing or radiation-blocking material, e.g. an enzyme which reacts with a substrate to produce a detectable material, such as a coloured material, in the detection zone.

25

#### Example

The purpose of this example is to confirm that the transmission reading system of the invention enables  
30 consistent data to be obtained from a testing device.

A dual-analyte testing device, selected at random from a batch of identical devices constructed as hereinbefore described with reference to Figures 1 and 2, using blue-  
35 coloured latex particles as a label concentrated in two test lines on a nitrocellulose strip to reveal the test result, was repeatedly inserted and "read" in a monitor

5 The slot incorporates a button or projection 305 which can fit into the depression 207 on the external face of the casing of the assay device. Precise positive location of the casing within the slot is therefore achieved. Because  
10 the depression is in a fixed position relative to the internal pin or peg 208 within the assay device, and hence the registration hole 112 in the assay strip 101, the two detection zones 102 and 103 on the strip are located in a precise position relative to the reading head. The hole in  
15 the assay strip therefore acts as a positive reference throughout the manufacture of the assay device and ensures that after the device has been used and presented to the monitor the detection zones on the strip will be in the same position relative to the reading head each time. Accordingly there is no need for the reading head to incorporate a scanning facility to locate the detection zones in each presented device.

20 The light source or illuminator 303 incorporates a plurality of LEDs 306 to generate light, and this shines onto the assay strip via a diffuser 307 and the observation window 209 in the lower half of the assay device casing. The light passes through the thin nitrocellulose strip 101 and exits the assay device through the result window 205 in  
25 the upper half of the casing. Immediately outside window 205 is a second diffuser 308. After passing through the second diffuser 308, the light encounters a plate 309 having a plurality of apertures 310-314. There are five apertures in total, two of which (311, 313) are adjacent to  
30 the detection zones and the others (310, 312 and 314) lie in positions on either side of these detection zone apertures. The apertures are of slit form corresponding to the detection lines on the strip. The width of each of the two apertures 311 and 313 corresponding to the detection  
35 zones themselves is double the width of each of the three other apertures, which act as controls.

correspond to feature 435 (Figure 4b), and feature 804 corresponds to feature 436 (Figure 4b).

5 Transmission spectrophotometry is a widely used technique for the quantification of dye concentrations in clear liquid solutions. Commercially available spectrophotometers generally require substantial modification to make measurements on diffuse (scattering) solutions. Transmission spectrophotometry is not generally  
10 thought of as an appropriate method of measuring highly diffuse samples so it is generally only adopted where an alternative approach cannot be applied. For the purposes of the invention, transmission measurement offers positive benefits over the more usual reflectance approach  
15 previously employed on test strips.

Some conventional strip assays employ reflectance measurement to assess dye concentration on the strip surface (e.g. glucose monitors). The chemistry of these  
20 assays occurs in a very thin layer on the surface of a test strip. In contrast, the chemistry of the preferred strip devices of the invention takes place throughout the thickness of the test strip. Because of variations in flow and reagent deposition, the concentration of detectable  
25 label captured at a reaction zone may differ according to depth.

Curvature, surface materials, finish and solvent effects may vary the ratio of specular to diffuse reflection. For  
30 reflectance measurements it is the diffusely reflected light from the surface of the strip that carries the signal information (i.e. that light will have interacted with the detectable label), whilst the specularly reflected light will contain no information (as this light is the component  
35 that has just bounced off the surface without interacting with the detectable label in the diffuse strip). Without resorting to relatively bulky and expensive systems, it is



The light passing through these apertures travels down a corresponding slot 315-319 in a baffle plate 320. At the far end of each slot is a light detector 321. The detectors 321 are of identical size and specification. At the front face 322 of the baffle plate 320, each slot is of the same size as the corresponding aperture. At the rear face of the baffle adjacent to the light detectors each slot is of the same size as the face of the light detector adjacent to it. Accordingly, the two slots (316, 318) associated with the detection zone apertures are parallel-sided. The three slots (315, 317 and 319) associated with the control apertures increase in size as they progress towards the light detector.

The slot in the monitor can also accommodate gripping or biasing means such as one or more spring-loaded plates or pins (not shown) to further enhance the positive location of the assay device within the slot.

Ideally, the same optical signal is derived from each aperture irrespective of the precise line position opposite the apertures. The apertures can be of different sizes to promote this objective. The dimensions of the reference zone should be chosen to correspond as closely as possible with the actual area of the detection zone on the strip.

To reduce the possibility of cross-talk between the apertures, the assay strip should be held as close as possible to the apertures when the assay device is located in the slot in the monitor.

As described above, there are five optical measurement channels in the reading device. In addition, there can be a sixth electronic reference channel that provides calibration of the electronic gains in the detector circuitry.

networks", can be used in place of conventional microprocessors based on "chip" technology.

5 As depicted in Figure 8, the combination essentially comprises a reading unit 800 to derive information from a test device, such as an assay strip, the reading unit comprising an illuminator 801 and a reader 802 (represented here as a photo diode). The reading unit feeds into a  
10 conversion unit 803 to convert the optical signal into a form usable by a microprocessor 804. As an optional feature, a calibration system 805 is provided to convert the signal derived from the reading unit into data corresponding, for example, to an absolute concentration value.

15 A timer, such as a clock 806 may be required to regulate measurements within a cycle. The microprocessor 804 processes, memorizes and interprets results in the light of previous events, particularly recorded from previous  
20 cycles. The user interface 807 will generally comprise at least means, such as a push button, which the user can operate at the commencement of a cycle to initiate the operation of the device as a whole. The power supply 808 should include means, such as a memory back-up capacitator  
25 809, to prevent loss of historical data when it becomes necessary to replace batteries.

Information can be conveyed to the user by means of a liquid crystal or LED display, for example. If desired,  
30 information on the state of fertility can be conveyed by a simple visual indication, eg a combination of colours showing, for example, green for infertile and red for fertile. Especially if the device is intended primarily as an aid to contraception, it should "fail safe" by showing  
35 a "fertile" signal.

As described above, features 803 and 806 together

5 A typical test strip may exhibit a gradient of detectable label concentration along its length, against which the detectable label at a reaction zone must be measured. To accommodate this measurements are ideally made either side of the reaction zone on the test strip. The signal from the reaction zone can be expressed as a ratio of the total signal recorded from the two adjacent reference areas on the strip.

10 The five measurement channels are divided into two reaction zones and three reference zones. One reference zone, located between the two reaction zones provides a reference optical measurement to both reaction zone measurements.

15 A reflectance measuring system must all be mounted on one side of the test strip. To achieve the same level of compactness for a five channel reading device would require the use of (relatively) expensive custom components. A transmission design can be made entirely from commercially-  
20 available, high volume optoelectronic components, facilitating the production of a monitor that is compact and relatively cheap.

25 The five detectors 321 are mounted on the back face of a baffle plate. Each detector views the test strip through an aperture in the baffle. The baffle prevents light viewed through one aperture from falling on adjacent detectors, and also provides accommodation for line placement tolerance. The position of the test zone within  
30 the field of view of a detector may vary from one edge of the aperture to the other in the x-axis. Any variation in the signal arising from this effect is a function of the angular displacement relative to the centre of the measuring detector. The depth of the baffle can be chosen  
35 to control the possible angular displacement of the test zone with respect to the detector, and to maintain the accuracy of the reading.

5 these two apertures are different and in particular the profile of the aperture 711 on the same face of the assay device as the conical hole 709 is shaped to match the profile of the projecting panel 507 covering the light sensors. This ensures that the reading head will only operate when the assay device is inserted in the correct orientation to ensure that the button 504 is depressed.

10 It will be appreciated that the overall layout and general shape of the monitor can be subject to very considerable variation from that described above without departing from the scope of the invention. The general shape and layout of the reading head is dictated by the need to cooperate effectively with the assay device but this shape can be  
15 varied considerably. The layout and nature of the user accessible controls and information display features can likewise be subject to considerable variation and are dictated to a large extent by aesthetic considerations.

20 The detailed electronics of a monitoring device capable of assimilating, remembering and handling analyte concentration data, as well as providing the preferred electronic features of the device discussed herein, and where appropriate predicting future events, such as the  
25 fertility status in an ovulation cycle on the basis of such data, can readily be provided by those skilled in the electronics art once they have been advised of the factors that such a device must take into consideration, and the information that the device must provide for the user. By  
30 way of example only, the basic functions that may be required in such a device are outlined in Figure 8 of the accompanying drawings and described briefly below. The individual features can be entirely conventional, and those familiar with the art of electronics will appreciate that  
35 other combinations and arrangements of such features can be employed to achieve the objectives of the invention. For example, so-called "hard-wired" systems, and "neural

The projection 305 is maintained in precise location with respect to the apertures. The reference pin locates into depression 207 in the test device casing. This depression is also precisely located with respect to the internal pin 208 moulded into the test device, on which the test strip is located by it's own locating hole punched through the strip. The reaction zones are precisely located with respect to the locating hole. In this manner, within manufacturing tolerances, the reaction zones are held in precise positions with respect to the apertures through which the detectors view the test strip.

The illuminator can consist of a series of LEDs embedded in or placed behind a diffusing medium which provides a uniform and diffuse illumination of the test strip covering the reference and signal zones.

The incorporation of a diffuser between the apertures and the test strip is beneficial for calibration purposes. In order to calibrate each of the optical channels in the absence of the test strip it is highly desirable that each detector is collecting light from the same areas of the illuminator as is the case when a test device is present. The diffuser can be selected to be the dominant diffuser in the optical path so that the introduction of the test strip does not contribute significantly to changes in the illumination distribution observed by the detectors. In addition, the diffuser element can enable the optical assembly to incorporate a 'wipe clean' surface, desirable for long-term repeated performance of the optical assembly. By modulating the intensity of the illuminator, the optical channels can be calibrated, without the aid of moveable parts, 'invisibly' to the user prior to the insertion of a test device.

The test strip can consist of an optically diffuse layer of nitrocellulose or the like, preferably sandwiched between

rear wall 505 of the slot and has sloping edges 508, 509 to give it a distinctive profile. At opposite ends of the front wall 510 of the slot are two pins (not seen in Figure 5) which are biased outwardly into the slot, e.g. by spring mechanisms contained within two housings 511, 512.

These same features are illustrated in Figure 6 which is a view directly downwards into the receiving slot. The two biased pins 600, 601 are seen. The purpose of these pins is to provide biasing means to push an inserted assay device against the rear wall 505 of the slot. If the receivable portion of an assay device has appropriately shaped holes or depressions to accommodate the fixed locating pin 506 and the projecting panel 507, the assay device can be pressed sufficiently closely to the rear wall of the slot to depress the button 504 and initiate the optical sensing procedure.

Figure 7 shows, in cross-section, part of an assay device 700 having a profile which can cooperate with the features seen in Figure 6. The assay device can be inserted into the slot with the broader central portion 701 abutting against shoulders 501, 502. The leading end 702 of the assay device has a slightly bevelled edge 703 to facilitate insertion into the slot past pin 600. The assay device comprises a hollow casing containing a porous assay strip 704 sandwiched between two sheets 705, 706 of transparent material. As described earlier, strip 704 is precisely located within the assay device casing by means of a pin 707 which extends through a hole 708 in the strip. On the outside of the assay device casing at a point corresponding to the centre of the locating pin 707 is a conical hole 709 which can accommodate the fixed locating pin 506 in the reader slot. Each side of the assay device casing has an aperture 710, 711 which, when the assay device is inserted in the slot correctly, will be adjacent the light source 443 and light sensors 444 respectively. The profiles of

- two layers of optically clear film, e.g. of polyester such as "Mylar". The clear film protects the nitrocellulose within which the assay reactions take place. Making reflectance measurements through thin transparent films is particularly difficult because of problems arising from specular reflections. Transmission measurement allows the optics to be constructed orthogonal to the measuring surface and minimises the adverse effects of reflection.
- 10 The invention is particularly applicable to the reading of test strips made of nitrocellulose and similar diffuse membranes that preferably do not exceed about 1 mm thickness.
- 15 Turning to Figure 4a, the monitor comprises a moulded casing, eg. of plastics material, having a generally oval rounded shape. The casing principally comprises an upper half 400 and a lower half, only the upper half of which is seen in Figure 4a. Towards the right hand side of casing 20 400 is a recess 401 having a backwardly sloping rear face 402. Rear face 402 incorporates an aperture 403 for a push button (not shown), a window 404 to reveal a display panel (not shown) and two windows 405 and 406 to reveal coloured lights or other indicators (again not shown) to convey 25 information to the user. Extending from the left end of recess 401 is a long slot 407 to provide access to a reading head (not shown). Recess 401 and slot 407 are closable by means of a lid 408 which is attached to the rear of the casing by two hinge points 409 and 410. The 30 upper surface 411 of casing 400 is recessed slightly to accommodate the lid when closed, so that the exterior of the closed device presents a relatively smooth continuous surface to the user. The lid can be flipped up to reveal the user-accessible features of the monitor. The lid is 35 closable by means of a spring clip (not seen in Figure 4a) which extends upwards through an orifice 412 in the front edge 413 of the casing. Front edge 413 of the casing

Turning to Figure 4c, the lower half 460 of the casing has an overall oval shape to match the upper half 400 and provides accommodation for the circuit board 430. The front edge 461 of the casing 460 accommodates a spring loaded catch 462 to fasten lid 408 when closed. Catch 462 is released by pressure on the front face 463 eg. applied by a finger tip. The floor 464 of the casing includes a battery chamber (beneath), and a small access hole 465 is provided towards the right hand end of the casing through which the battery connector 439 can be passed and linked to batteries 466. The batteries are retained by a cover 467 which can be clipped to the underside 468 of the casing.

The constituent parts of the casing can be moulded from high impact or similar plastics materials such as polystyrene and polycarbonate and held together by "push fit" clips or threaded screws or any other appropriate mechanism.

Turning to the enlarged illustration of the reading head, as seen in Figure 5, the slot 442 for receipt of an assay device is of parallel sided form, but its width is enlarged at its right hand end 500 in a stepped manner to provide a pair of shoulders or abutments 501, 502 against which a correspondingly enlarged portion of an assay device can be abutted. This can facilitate effective insertion of an assay device into the reading head. Within the narrower working part 503 of the slot is a button 504 mounted on the rear wall 505 of the slot, which must be fully depressed to activate the reading mechanism. Appropriate insertion of a testing device causes adequate depression of this button.

Also on the rear wall 505 of the slot is a fixed locating pin 506 which must engage with a corresponding hole in an inserted assay device. Also on the rear wall 505 is a light-transmitting panel 507 which covers the optical sensors. Panel 507 extends outwardly beyond the plane of



incorporates a further orifice 414 through which a further indicator light (not shown) may be revealed.

5 Turning to Figure 4b, the circuit board 430 is of rounded rectangular shape to match the interior shape of the casing, and carries all of the operational features of the monitor. These include a push button 431 which the user can press to initiate the monitoring of an ovulation cycle. When the circuit board is mounted within the casing and covered by upper half thereof, the push button is accessible through aperture 403. To the right of the push button is a visual display panel 432 such as a liquid crystal display which is visible to the user through window 10 404. To the right of the display panel are two light guides 433 and 434 which transfer, for example, coloured light (such as red and green) from two LEDs or similar lamps (not shown). Appropriate "chips" and memory circuits 15 435, 436 are mounted on the circuit board. A further light guide 437 mounted at the front edge 438 of the circuit board can convey light from another LED (not shown) to 20 aperture 414. This light may indicate, for example, to the user that an assay is required. This light can be a different colour from the lights associated with display panel, eg. yellow. A battery connector 439 hangs from 25 beneath the circuit board for connection to batteries retained in the lower casing (see Figure 4c). Also at the front of the circuit board is a switch 440 operable by the spring catch of lid 408.

30 At the left hand end of the circuit board is mounted the reading head 441 which comprises a central receiving slot 442 to accommodate one end of an assay device (not shown). On the front of receiving slot 442 is an illuminator 443 and immediately opposite at the rear of the slot is an 35 optical sensing system 444 so that light can be passed across the slot (and through a testing device when inserted) and evaluated by the sensor.